

# ORAL FLUID TEST

## STAT<sup>+</sup> SWAB II



### STATSWAB<sup>®</sup> II

The STATSWAB<sup>®</sup> II is a NEW and INNOVATIVE, fully integrated oral fluid drug screen device. The STATSWAB<sup>®</sup> II is the simplest and fastest oral fluid drug screen on the market. Simply swab the mouth and close the cap. It's that easy! See back for details.

- Fast
- Accurate
- Reliable
- Easy-to-Use
- Affordable
- Dark Lines

**CALL FOR A  
FREE SAMPLE!**

### TEST FEATURES

- Fully Integrated
- Simple Mouth Swab
- No Steps to Activate
- Observable
- No Restroom Needed
- Test Up to 14 Drugs
- Transport Sample to Lab
- Flat-Sided for Photocopying

### TEST AVAILABLE

#### Drugs of Abuse:

Marijuana	Methadone
Cocaine	Buprenorphine
Opiates	Ecstasy
Phencyclidine	K2/Spice
Methamphetamine	Cotinine
Amphetamine	Propoxyphene
Benzodiazepines	Alcohol
Oxycodone	
Barbiturates	

The STATSWAB II is for forensic use only. Not intended for treatment or diagnostic purposes.



**Toll Free: 1-800-668-0031**

[www.Tryrapid.com](http://www.Tryrapid.com)

# STAT<sup>+</sup> SWAB<sup>II</sup>

## EASY-TO-USE

## FAST

## ACCURATE

CALL FOR A FREE SAMPLE!



NEW!


# STAT<sup>+</sup> SWAB PLUS<sup>+</sup>

### Interpreting Alcohol Test Results

1. Read Results at 2 Minutes
2. Compare Reactive Pad to Color Blocks Below:
3. Interpretation:

**NEGATIVE** - No color changes on reactive pad.  
**POSITIVE** - Reactive pad changes color. Estimate the approximate blood alcohol level by comparing the color of the reactive pad to the color chart below.

### Approximate Blood Alcohol Level

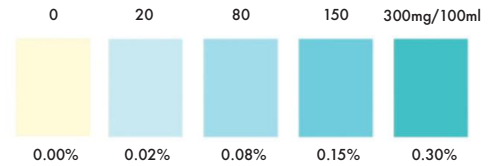

## PROCEDURE

Allow the test device to reach room temperature [15-30°C (59-86°F)] prior to testing. Do not place anything in the mouth including food, drink, gum, or tobacco products for at least 10 minutes prior to collection of oral fluid specimen.


### STEP 1

Remove the collection stick and test tube from the sealed pouch.




### STEP 2

Tear off the package of the collection stick.



### STEP 3

Insert the sponge end of the collection stick into mouth and soak sponge into saliva for 3 minutes. (Note: Time should be longer for people of little saliva. If the amount of saliva pressed into the test tube is not adequate for testing, collect more with another new collection stick and express the saliva into tube again.)



### STEP 5


Press down the lid to close the test tube. Keep the test tube vertically until you begin to read the test results.



### STEP 6

#### INTERPRETING RESULTS

Read results at 10 minutes. (If there is a label over reading window, peel off the label to read test results.) Do not read results after 1 hour.



### STEP 4

Hold the test tube vertically and place the collection stick with saturated sponge into the test tube. Make sure to fit the groove of collection stick onto the guide rail of test tube and press the collection stick to full extent.



Phone: 1-800-668-0031

Rapid Response Drug Testing